


**Meas.Nr.** 63935      **Date** Montag, 13 Mai 2013 02:52      **Personal Report No.:**  
**Material** Glass V3      30min P6cl 80 ml ZrO2 5mm      **M130105**  
**Description** pre dispersed in 0,1% Na4P2O7 + 1min LABORETTE 17 ultrasonic

**Calculation** Fraunhofer      broad      **TradeOff** 1.000000e+003  
**Scans Fine** 100      **Scans Coarse** 100      **Channels** 102      **Beam Obscuration** 14.00 %  
**Meas. Range** 0.08 [µm] - 2000.00 [µm]      **Pump** 7      **Ultrasonics** 10

%	< µm
5	0.54
10	0.71
15	0.86
20	1.03
25	1.19
30	1.37
40	1.79
50	2.30
60	2.99
70	3.95
80	5.38
90	7.85
95	10.16
98	12.85
99	14.69

%	< µm
19.2	1.0
44.4	2.0
65.8	3.5
77.8	5.0
85.3	6.5
90.4	8.0
94.7	10.0
97.7	12.5
99.1	15.0
99.7	17.5
100.0	20.0
100.0	22.5
100.0	25.0
100.0	27.5
100.0	30.0

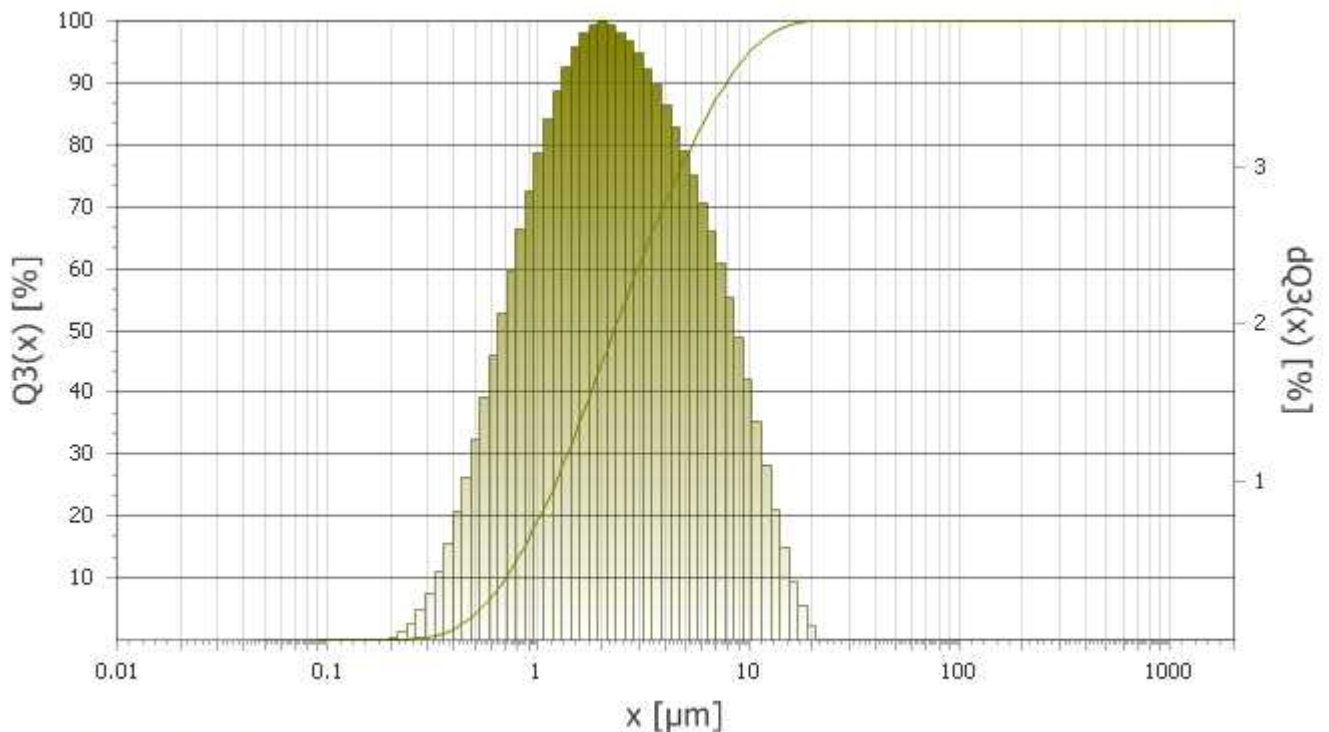

▲ 63935 dQ3(x) — 63935 Q3(x)