


Mess.Nr. 69559 **Datum** 10/29/2013 15:06 **Bearbeitungs-Nr:**
Material Kalk-Natron-Glas-Glas (MTP-Messung) Mie Neuberechn. 90min P7pl 0,5 mm ZrO2 **M130270**
Bemerkung in Wasser + 0,1% NA4P2O7, ohne US

Berechnung Mie n = 1.54429 -i 0 **TradeOff** broad (100.0)
Scans 100 **Scans** 0
Feinbereich **Grobbereich**
Messbereich 0.08 [μ m] - 42.30 [μ m] **Messkanäle** 57 **Strahlabsorption** 15.00 %
Pumpe 5 **Ultraschall** 10

%	< μ m
5	0.089
10	0.095
15	0.103
20	0.112
25	0.122
30	0.133
40	0.158
50	0.188
60	0.229
70	0.284
80	0.371
90	0.553
95	0.803
98	1.452
99	1.904

%	< μ m
6.3	0.08
6.7	0.09
13.1	0.10
37.1	0.15
53.2	0.20
64.3	0.25
72.3	0.30
82.2	0.40
88.0	0.50
91.4	0.60
95.0	0.80
96.5	1.00
100.0	5.00
100.0	8.00
100.0	10.00

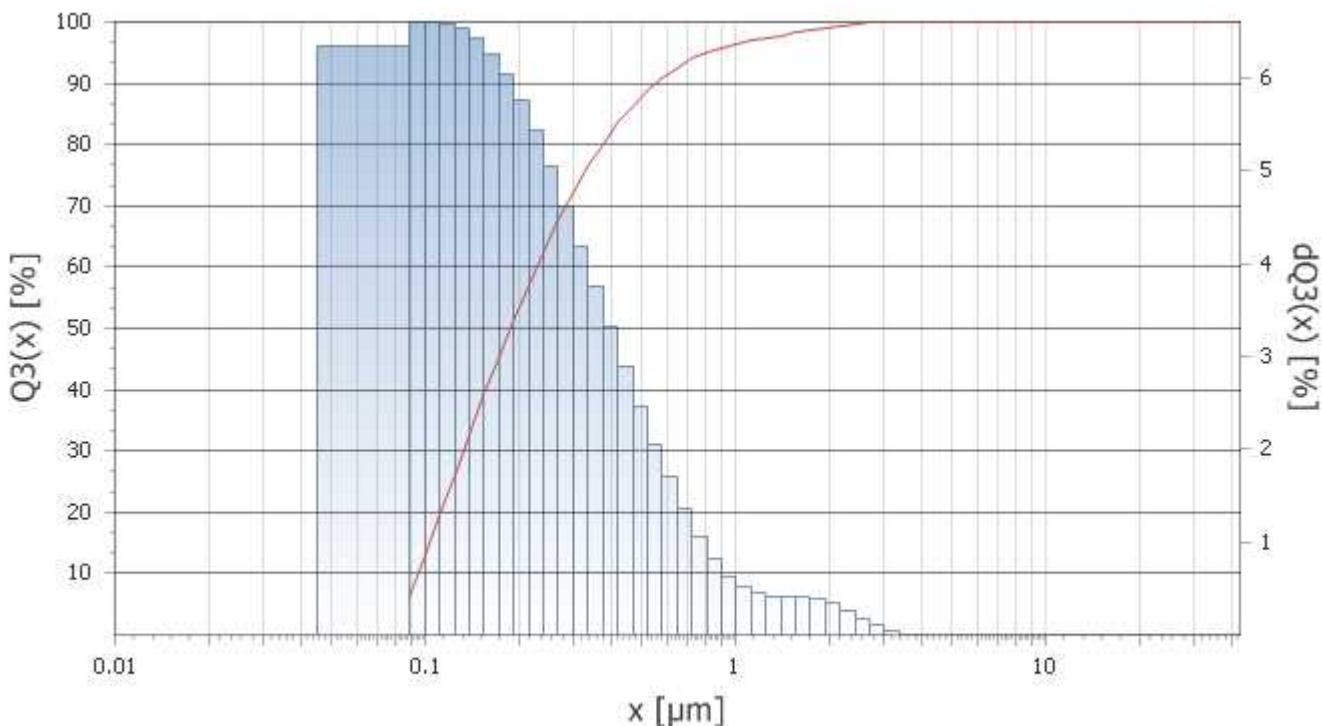

▲ 69559 dQ3(x) — 69559 Q3(x)