


Mess.Nr. 71458 **Datum** 12/17/2013 13:17 **Bearbeitungs-Nr:**
Material Leucit 3h P7pl 0,1 mm ZrO2 **M130305**
Bemerkung in Wasser + 0,1 % Na4P2O7 - 2 min Ultraschallbad LABORETTE 17

Berechnung Mie n = 1.52510 -i 0 **TradeOff** broad (100.0)
Scans 100 **Scans** **Messkanäle** 108 **Strahlabsorption** 5.00 %
Feinbereich **Grobbereich** 0
Messbereich 0.01 [µm] - 42.30 [µm] **Pumpe** 3 **Ultraschall** 10

%	<µm
5	0.013
10	0.021
15	0.053
20	0.064
25	0.073
30	0.082
40	0.098
50	0.116
60	0.136
70	0.161
80	0.195
90	0.250
95	0.302
98	0.367
99	0.415

%	<µm
2.5	0.01
9.8	0.02
10.6	0.03
13.7	0.05
29.0	0.08
41.0	0.10
81.2	0.20
94.9	0.30
98.8	0.40
99.7	0.50
99.9	0.60
99.9	0.70
99.9	0.80
99.9	0.90
99.9	1.00

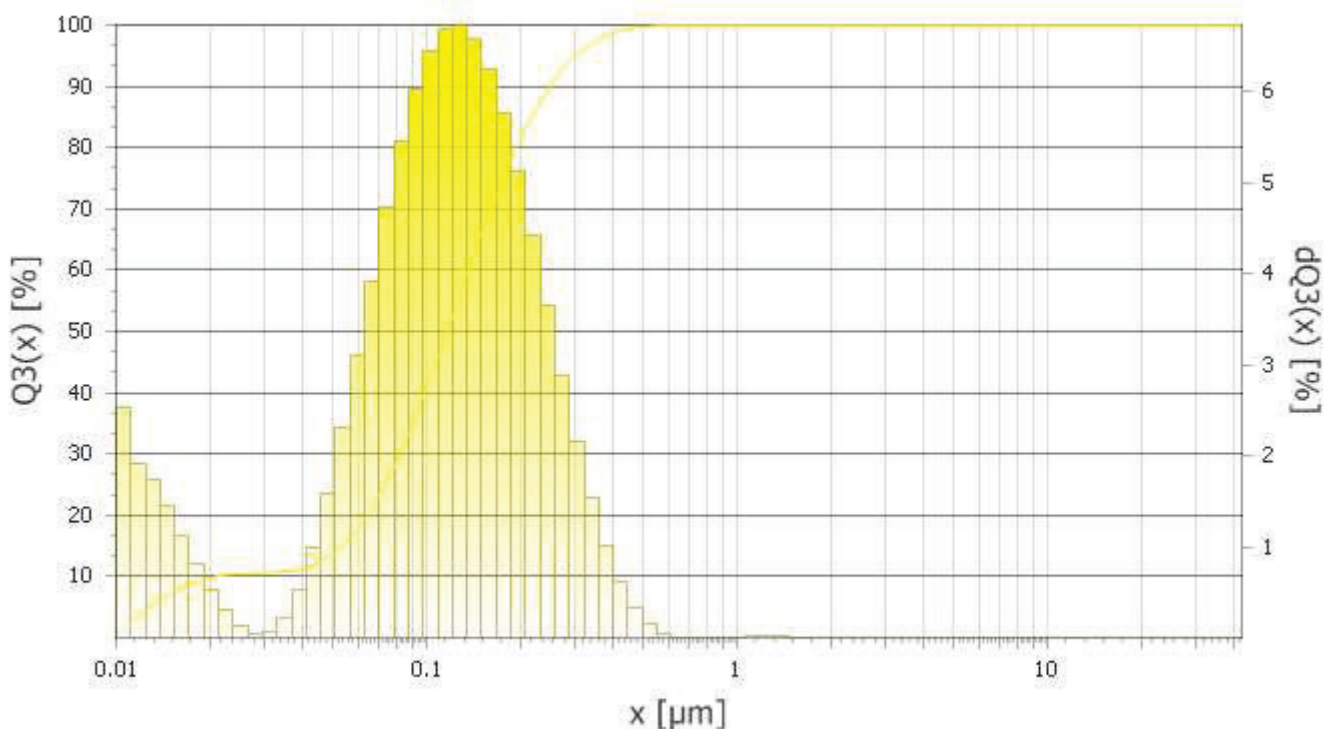

▲ 71458 dQ3(x) — 71458 Q3(x)